

Tissue doppler imaging

Volume 3 Issue 4 - 2015

Hesham Khalid Rashid Mousa

Department of Cardiology Medicine, Benha university, Egypt

Correspondence: Hesham Khalid Rashid Mousa, Department of Cardiology Medicine, Benha university, Egypt, Tel 20482578334, Email hesham_mosa2001@yahoo.com**Received:** June 13, 2015 | **Published:** October 12, 2015**Keywords:** tissue doppler imaging

Introduction

Echocardiography is now the method more commonly used for assessment of diastolic function. In addition to high-resolution 2-D images, Doppler flow velocity offers important information about the dynamics of ventricular filling. Pulsed wave Doppler of the mitral and pulmonary veins is used for routine assessment of left ventricular diastolic function. Similarly, Doppler flow of the tricuspid and hepatic veins is used to evaluate right ventricular diastolic function.¹ An important limitation of the spectral Doppler assessment of diastolic function is its dependence of loading conditions. With worsening left ventricular diastolic function there is a compensatory increase in left atrial pressure, increase in the velocity of the E wave of the mitral inflow and pseudonormalization of the filling pattern (normal E/A ratio and deceleration time), TDI can differentiate in this case between normal and pseudonormal pattern.² Recently, 2 new technologies, color M-mode and Doppler Tissue echocardiography, have emerged that are very promising in complementing the information provided by Doppler echocardiography and may allow us a more complete evaluation of diastolic function.³

Principle of TDI

Tissue Doppler scanner is operated in a similar way to conventional ones. Most of the system parameters and their effects on the image are exactly the same, as:⁴

Frame rate/Field of view: The frame rate is indirectly controlled through the definition of the region of interest. The framing rate is an important factor in determining the acceptability of 2-D cardiac images. In conventional color Doppler flow imaging systems, the frame rate is usually set 10 frames/second with pulse repetition frequency of 4.5 KHz. However, under these conditions, a time lag can occur between the beginning and the end of the scanning of one frame and 100 ms is needed, which was provided an insufficient temporal resolution in TDI for accurate depiction of each phase of myocardial motion⁵. For one frame to be completed and starting another frame, it is possible to reduce the time lag for each frame thus allowing increasing the framing rate. In TDI, the numbers of data samples were reduced to half that of the conventional color flow imaging system. The pitch of the scanning line was also expanded to 1.5times that of the conventional system. All these modifications allowed the use of smaller packet sizes and higher pulse repetition frequencies that resulted in framing rate up to three times that of the conventional color flow.

Gate size: Increasing the gate size will lead to increase sensitivity (the ability to detect moving tissue) but with decreased spatial resolution due to a higher sample volume size.⁶

Gain setting: In TDI system three gain settings interact to produce the image, the gray scale-depth adjustable gain, the Doppler gain and the TDI gain. The relative amount of gray 2D and color information depend on all these settings. To increase the amount of color it is necessary to increase the Doppler gains or to decrease the (global or

regional) 2D gain. Incorrect settings may produce poorly colored or saturated images.⁷

Scale: The range may be selected to display the lower and higher velocities. As in conventional Doppler imaging, the most expanded but still aliasing-free scale should be selected.

Color map: Usually the color defines the direction however color saturation and or hue indicates the velocity of the motion. Many different color maps exist, they may be liner or non-liner, and even a given interval may be selected for tagging a different color.

Persistence: The image may be either temporally or spatially smoothed to produce better looking of the image.

Low velocity filtering: Lowest velocity signals can be rejected, thus improving the signal to noise ratio.

Threshold filter: It allows the exclusion of the weakest signals, which may be largely noisy.

Transmitter power: Color Doppler and 2D power may be independently set in some systems.

All these settings and some others contribute to image quality and interact with each other. These parameters must be adjustable so that we can obtain the optimal image quality. Also tissue Doppler shares the same limitation that of flow Doppler, the most important of which is angle dependence. But there are two major differences between the acoustic characteristics of Doppler signals from the cardiac wall and those from blood flow⁸:

- a. Wall motion velocity is much slower than blood flow velocity (usually 10 cm/s) whereas blood flow velocity in the ventricular cavity is approximately (10-100cm/s).

- b. Doppler signal intensity of wall motion is much greater (about 40 db) than that of Doppler signal coming mainly from red blood cells, so it is possible to obtain images of tissue Doppler motion of high resolution without significant artifact originating from blood pool. In such images, each pixel displays one color representing a mean velocity value.⁹

Doppler echocardiography relies on detection of the shift in frequency of ultrasound signals reflected from moving objects. With this principle, conventional Doppler techniques assess the velocity of blood flow by measuring high-frequency, low-amplitude signals from small, fast-moving blood cells. In TDI, the same Doppler principles are used to quantify the higher-amplitude, lower-velocity signals of myocardial tissue motion⁵ (Figure 1).

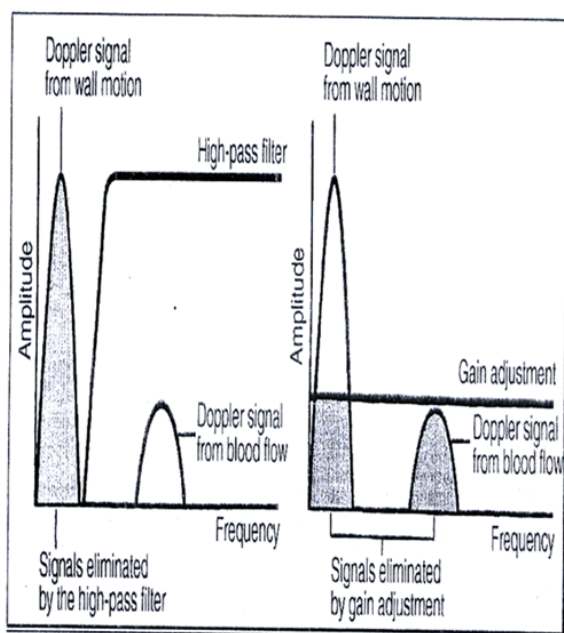


Figure 1 The higher-amplitude, lower-velocity signals of myocardial tissue motion.

In a conventional Doppler system a high pass filter is incorporated to eliminate these low velocity signals and the gain settings are increased to amplify the signals reflected by moving blood. To display tissue velocities, two relatively simple alterations in Doppler signal processing are required:

- The high pass filter is bypassed and
- Lower gain amplification is used to eliminate the weaker intensity blood flow signals.¹⁰

TDI modes

Color TDI: In conventional echocardiography Doppler signals from red blood cells are detected at each sampling site along the ultrasound beam. The frequency shift is measured and converted into a digital format. By autocorrelation method different velocities are correlated with a preset color scheme and, superimposed on the 2-dimensional image displayed as color flow on the monitor. Blood flow towards the transducer is color coded in red shades while blood flow away from the transducer is color coded in shades of blue. Velocities exceeding the Nyquist limit lead to aliasing and to reversal of color and variant colors respectively. In TDI, the same principles have been applied. The upper limit of measurable velocities is determined by the pulse repetition frequency, which is also the sampling frequency.¹¹ With the latest techniques, frame rates of up to 240/s can be obtained. Because

ventricular wall motion velocity at rest is about 10cm/s or less and increases up to 15 cm/s during stress aliasing is unlikely under these conditions. As for pulsed wave and continuous Doppler, Doppler shift and hence temporal and spatial resolution are dependent on frame rate which itself is correlated to probe frequency, pulse repetition frequency and sector angle.¹²

Clinical applications of color-coded TDI: No information regarding wall motion velocity can be obtained from the stop-frame images of conventional two-dimensional echocardiography. In contrast, color-coded TDI, in which wall motion velocity is superimposed on the two-dimensional echocardiography, permits visual assessment of wall motion velocity in real time. Therefore, it is possible to estimate the wall motion from both wall configuration and motion velocity.¹³ With the present system, serial changes in the ventricular wall motion over time can be analyzed, particular with the use of M-mode color-coded tissue Doppler imaging. This ability may be applicable to detection of sites of early ventricular contraction associated with accessory pathways in patients with the Wolff-Parkinson-White syndrome.¹⁴

Pulsed- Wave Tissue Doppler Imaging (PW-TDI): This is the easiest way to measure myocardial velocities and has been used for interrogation of myocardial or mitral annular velocities. Using this modality a sample volume is placed in the ventricular myocardium immediately adjacent to the mitral annulus and a spectral display is obtained.¹⁵

Technical issues associated with TDI: Certain pitfalls, which may affect or influence the Doppler signals:

- Sample volume size and positioning
- Doppler gain
- Mitral annular calcification
- Phase of respiration
- Beam alignment

Gain: Gain can affect the peak Doppler tissue velocities. Therefore, gain should be minimized to allow for clear Doppler signals with minimal background noise.¹⁶

TDI annular site: Although the E/E' ratio was the single best parameter for predicting mean left ventricular diastolic pressure (LVDP) for all levels of systolic function, Ommen et al.,¹⁷ demonstrated that E/E' ratio using the medial annulus correlated better with mean LVDP.¹⁷ However, a recent publication showed that the lateral annular E' velocities used for the E/E' ratio correlated best with LAP when the EF is greater than 50%; if the EF was less than 50%, a combination of conventional and refined Doppler indices may be used without significant error.¹⁸

Phase of respiration: The phase of respiration affects TDI recordings in view of breathing-associated shifts in cardiac position. When possible, the sonographer should obtain lateral TDI during end expiratory apnea, to improve accuracy and consistency of the peak TDI velocities.

Sample volume size and location: Placement at the annulus is critical to produce accurate Doppler tissue tracings. Subtle changes in sample volume positioning outside the annulus can highly influence the Doppler tracings.¹⁹ The septal annulus has been reported to have less excursion, resulting in lower velocities than the lateral annulus.²⁰ Therefore, different sample volume size should be used for different annular location (lateral vs septal; septal annular imaging may improve with an approximate 3.5mm sample volume, and lateral annular

imaging improved with an approximate 5.0mm sample volume). The rationale behind using different sample volume size is that increased lateral annular motion may require a larger sample volume to record the annular velocities properly. To optimize all components of the TDI signal, sample volume size should be proportional to annular motion and not limited to either septal or lateral annulus.²¹

Mitral annular calcification: Mitral annular calcification (MAC) may influence annular motion by reducing its excursion. Soeki et al.,²¹ has shown that severe MAC is associated with elevated trans-mitral inflow velocities in the absence of significant valvular stenosis, and low E' velocities. Thus, for patients with extensive MAC, the E/E' ratio may be elevated. Whether elevation in this ratio reliably reflects elevated LAP has not been completely established by hemodynamic validation studies. Until further data is furnished on MAC and the estimation of early diastolic filling pressures, the sonographer should use caution when reporting the E/E' ratio.²¹

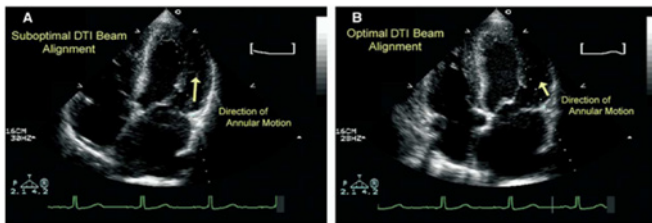


Figure 2 Suboptimal and optimal annular Doppler tissue imaging (TDI) beam alignment. **A:** Large angle of insonation (increased cosine) between Doppler beam and lateral annulus. As with other Doppler techniques, large insonation angle (cosine > 20 degrees) can lead to significant underestimation of annular velocities. **B:** in same patient, Doppler beam aligned more parallel (cosine < 20 degrees) to motion of mitral annulus. Alignment will result in more accurate recordings of annular velocities.²¹

Systematic approach for acquiring accurate TDI waveforms:¹⁵

The Sonographers Check list for more accurate and reproducible TDI. The following is a systematic approach that can guide the sonographer to obtain more accurate and reproducible annular Doppler tissue tracings:

1. Determine if the ultrasound manufacturer has preset Doppler tissue settings.
2. Optimize the apical 4-chamber view by aligning the cursor as parallel as possible through the annulus to avoid possible underestimation of the Doppler signal; an angle of insonation less than 20 degrees parallel to annular plane will allow for more accurate Doppler velocities.
3. Sample volume size should be adjusted proportionally to annular motion: use a sample volume of approximately 3mm for the septal annulus and 5mm for lateral annulus. Carefully visualize the sample volume relative to annular motion and increase or decrease the sample volume size accordingly.
4. Once the Doppler cursor is aligned optimally, activate the Doppler tissue preset. Decrease the Doppler scale to less than 25cm/s for better visualization of the peak annular velocities. A sweep speed between 50 and 100 mm/s is adequate for measurement of peak annular velocities.
5. Ask the patient to breathe in, breathe out, and then hold their breath at the end of expiration. Carefully reposition the sample volume directly into the selected portion of the annulus. Activate pulsed wave Doppler tissue. Peak TDI wave form velocities should be uniform, consistent, with little or no beat-to-beat variation of the peak velocities (Figure 2).

Reproducibility of TDI: To date, few studies have reported on the reproducibility of annular TDI. Vinereanu et al.,²² showed the best inter observer reproducibility of annular diastolic velocities when obtained from the lateral mitral annulus. Special attention to technical factors along with more accurate Doppler beam alignment perpendicular to the annulus may increase reproducibility.²²

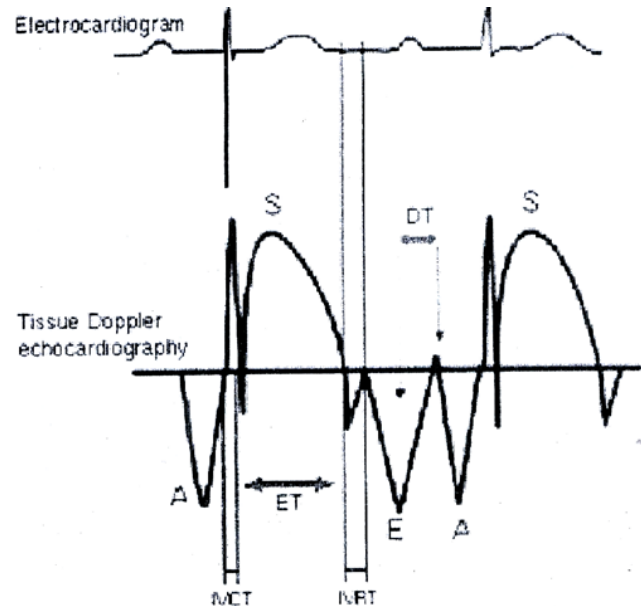


Figure 3 Tissue Doppler time intervals and velocities measured from lateral mitral annulus. IVCT: isovolumic contraction time; IVRT: isovolumic relaxation time; S: the main systolic velocity; E: the early diastolic velocity; A: the late diastolic velocity; ET: ejection time; DT: E-wave deceleration time.²⁴

Normal pattern of pulsed wave TDI (Figure 3):¹⁰ From the velocity curve the following velocity waves can be identified:

- a. Isovolumic contraction wave (IC-wave): This is biphasic wave (Ica & ICb) representing the isovolumic contraction phase (starts with Q-wave).
- b. Systolic wave: Large systolic wave occurs after (r-wave on ECG and extends to the end of the T-wave). Its peak velocity ranges from 8-18 cm/sec; it is usually positive wave except for the anterior wall and the septum in the parasternal views. The six-site average for peak systolic mitral annular velocity by pulsed wave TDI method of greater than 7.5 cm/sec is predictive of an ejection fraction greater than 50% with 88% sensitivity and 97% specificity.²³
- c. Iso volumic relaxation wave: It starts from the end of the S-wave to the beginning of E-wave. The IVRT in healthy normal subjects ranges 35 ± 15 sec to 76 ± 25 sec with mean value of 52 ± 15 m sec, there is some degree of heterogeneity being lower at the basal than at distal segments. This wave is biphasic wave IRa is the positive component. IRb is the negative component.
- d. Early Filling phase (ETDI): It coincides with the trans-mitral E-wave but peaks earlier than that of mitral flow. It ranges in normal subjects from 10 ± 3 cm/sec to 14.8 ± 3.9 cm/s. Also there is some heterogeneity of the peak ETDI from basal to mid and apical segments. It is usually negative wave except for the septum and anterior wall. The peak early diastolic velocity is blunted with restrictive cardiomyopathy and preserved constrictive pericarditis.²³

- e. Late Filling phase (ATDI): It follows the P-wave of ECG. Its normal values ranges from 5.8 ± 2.4 cm/s with some heterogeneity between different myocardial segments.
- f. E' TDI/A' TDI ratio: It is the most sensitive important index of ventricular diastolic function. It ranges normally from 1.9 ± 0.9 to 3 ± 1.4 and correlates directly with the global E/A ratio: Alteration of left ventricular global diastolic filling depends on the magnitude and extension (number of segments) of regional diastolic dysfunction¹.
- g. The biphasic signals during the isovolumic phases (contraction and relaxation) are low in velocity and of very short duration and they were considered due to muscular elasticity or translation of the heart during these phases of the cardiac cycle when pressure gradients act as constant left ventricular volumes. They are highly variable and therefore these waves are not included in the data analysis as the other three distinct deflections (S, E' and A' waves).²

Acknowledgments

None.

Conflicts of interest

Author declares there are no conflicts of interest.

References

1. Sohn D, Chai I, Lee DJ, et al. Assessment of mitral annulus velocity by Doppler tissue imaging in the evaluation of left ventricular diastolic function. *J Am Coll Cardiol.* 1997;30(20):474-480.
2. Galiuto L, Ignone G, DeMaria A. Contraction and relaxation velocities of the normal left ventricle using pulsed-wave tissue Doppler echocardiography. *Am J Cardiol.* 1998;81(5):609-614.
3. Labovitz A, Pearson A. Evaluation of left ventricular diastolic function: clinical relevance and recent Doppler echocardiographic insights. *Am Heart J.* 1998;114(4 pt 1):836-851.
4. Mundigler G, Zehetgruber M. Tissue Doppler Imaging: Myocardial Velocities and Strain – Are there Clinical Applications? *J Clin Basic Cardiol.* 2002;5(2):125-132.
5. Price D, Wallbridge D, Stewart M. Tissue Doppler imaging: Current and potential clinical applications. *Heart.* 2000;84 Suppl 2:11-18.
6. Lars-Åke B, Anna B, Kambiz S. Clinical Physiology and Functional Imaging. 2004;24(3):147-155.
7. Ingul C, Torp H, Aase S, et al. Automated analysis of strain rate and strain: feasibility and clinical implications. *J Am Soc Echocardiogr.* 2005;18(5):411-418.
8. Evans D, McDicken M, Skidmore R. Doppler ultrasound: physics, instrumentation and clinical application. Chichester: *John Wiley and Sons.* 1993.
9. Urheim S, Edvardsen T, Torp H, et al. Myocardial strain by Doppler echocardiography. Validation of a new method to quantify regional myocardial function. *Circulation.* 2000;102:1158-1164.
10. Garcia-Fernandez M, Zamarrano J, Azevedo. Normal pattern with Doppler tissue imaging echocardiography. *MC Grow Hill.* 1998. P. 23.
11. Erbel R, Nesser H, Drozd J. color coded tissue Doppler echocardiography a new method for quantitation of cardiac wall motion (abstract). *Eur J Cardiol.* 1997;1997:42-48.
12. Miyatake K, Yamagishi M, Tanaka N, et al. New method for evaluating left ventricular wall motion by color-coded tissue Doppler imaging: in vitro and in vivo studies. *J Am Coll Cardiol.* 1995;25(3):717-724.
13. Simpson J. Echocardiographic assessment of long axis diastolic function: a simple solution a complex problem. *Heart.* 1997;78(3):211-212.
14. Zamorano J, Wallbridge D, Ge J, et al. Non-invasive assessment of cardiac physiology by tissue Doppler echocardiography. A comparison with invasive haemodynamics. *Eur Heart J.* 1997; 18(2):330-339.
15. Gaso P, Sutherland C, Fleming A, et al. Doppler tissue imaging: current status and future prospects. *Ital Cardiol.* 1995;25(5):636-647.
16. Rodriguez L, Garcia M, Ares M, et al. Assessment of mitral annular dynamics during diastole by Doppler tissue imaging: comparison with mitral Doppler inflow in subjects without heart disease and in patients with left ventricular hypertrophy. *Am Heart J.* 1996;131(5):982-987.
17. Ommen S, Nishimura R, Appleton C, et al. Clinical utility of Doppler echocardiography and tissue Doppler imaging in the estimation of left ventricular filling pressures: a comparative simultaneous Doppler catheterization study. *Circulation.* 2000;102(15):1788-1794.
18. Rivas-Gotz C, Manolios M, Thohan V, et al. Impact of left ventricular ejection fraction on estimation of left ventricular filling pressures using tissue Doppler and flow propagation velocity. *Am J Cardiol.* 2003;91(6):780-784.
19. Dumesnil J, Gaudreault G, Honos G, et al. Use of Valsalva maneuver to unmask left ventricular diastolic function abnormalities by Doppler echocardiography in patients with coronary artery disease or systemic hypertension. *Am J Cardiol.* 1999;68(5):515-519.
20. Nagueh S, McFalls J, Meyer D, et al. Tissue Doppler imaging predicts the development of hypertrophic cardiomyopathy in subjects with subclinical disease. *Circulation.* 2003;108(4): 395-398.
21. Hill JC, Palma RA. Doppler Tissue Imaging for the Assessment of Left Ventricular Diastolic Function: A Systematic Approach for the Sonographer. *J Am Soc Echocardiogr.* 2005;18(1):368-380.
22. Vinereanu D, Khokhar A, Fraser A. Reproducibility of pulsed wave tissue Doppler echocardiography. *J Am Soc Echocardiogr.* 1999;12(6):492-499.
23. Gorcsan J, Gulati V, Mandarino W, et al. Color-coded measures of myocardial velocity throughout the cardiac cycle by tissue Doppler imaging to quantify regional left ventricular function. *Am Heart J.* 2000;131(6):1203-1213.
24. Cui W, Roberson D, Chen Z, et al. Systolic and diastolic time intervals measured from Doppler tissue imaging: Normal values and Z-score tables, and effects of age, heart rate, and body surface area. *J Am Soc Echo-cardiogr.* 2008;21(4):361-370.